



Patient ID <b>SA00063200</b>	Patient Name <b>TESTINGRNV, HCVQU4</b>	Birth Date <b>1983-01-01</b>	Gender <b>M</b>	Age <b>30</b>
Order Number <b>SA00063200</b>	Client Order Number <b>SA00063200</b>	Ordering Physician <b>Client, Client</b>	Report Notes	
Account Information <b>C7028846 DLMP Rochester</b>		Collected <b>10 Oct 2013 00:00</b>		

**HCV RNA Detect/Quant, S**

**Undetected IU/mL**

Result in log IU/mL is Undetected.

**ADDITIONAL INFORMATION**


The quantification range of this assay is 15 to 100,000,000 IU/mL (1.18 log to 8.00 log IU/mL). Testing was performed by the COBAS AmpliPrep/COBAS TaqMan HCV Test, version 2.0 (Roche Molecular Systems, Inc.).

**Received:** 11 Oct 2013 11:29

**Reported:** 11 Oct 2013 11:47

**SDL**

**Reference Value**  
Undetected

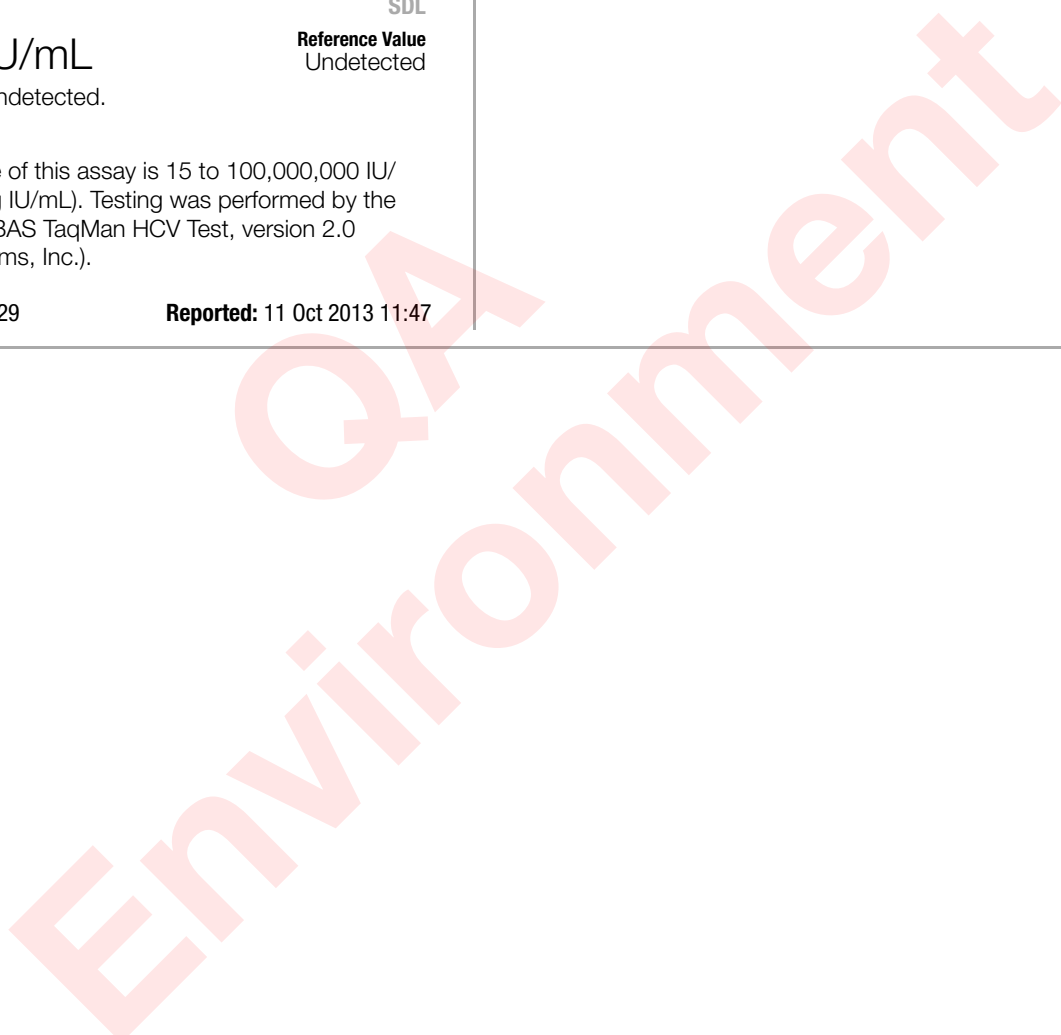

**Performing Site Legend**

Code	Laboratory	Address
SDL	Mayo Clinic Laboratories - Rochester Superior Drive	3050 Superior Drive NW, Rochester MN 55901